

## EDI™ MAHA ELISA Kit

Enzyme Linked ImmunoSorbent Assay (ELISA) for the measurement of Mouse Anti-Human Antibody (MAHA) Level in Serum and Plasma

REF **KT 807**



96



For Research Use Only

Not for Use in Diagnostic Procedures

### INTENDED USE

This ELISA (enzyme-linked immunosorbent assay) kit is produced for the quantitative determination of mouse anti-human antibody (MAHA) levels in mouse serum or plasma samples. It detects both MAHA-IgG and MAHA-IgM subtypes. The test is used for detection of mice with positive MAHA that may affect prescribed studies involving humanized monoclonal antibody, which is essential to avoid misleading immunoassay test results and conclusion.

This kit can also be used for specimens collected from other animals such as rat, dog, cat, rabbit, primate, etc.

### SUMMARY OF PHYSIOLOGY

Development of humanized monoclonal antibodies (IgG) and their fragments as *in vivo* diagnosis procedure (radionuclides) and treatment for patients with various diseases has made great progress. In animal study, even a single dose injection of a humanized monoclonal antibody or its fragment may induce immune response directed against this foreign protein (immunogen). In the circulation, the presence of mouse antibody against human antibody would bind to the injected humanized antibody therapeutics or diagnosis and diminish the efficacy of either *in vivo* diagnosis or treatment. The present of MAHA in mouse serum or plasma specimens may cause both false positive and false negative immunoassay test results depending on assay principles and monoclonal/polyclonal antibodies used in the assay system.

Therefore, the presence of MAHA would eventually lead to unreliable pre-clinical data collection and study conclusion.

This MAHA ELISA is a ready-to-use test kit with well-breakable microtiter plate and simple test procedures. It also provides a wide measurement range without high dose "hook" effect.

### ASSAY PRINCIPLE

This ELISA is designed, developed and produced for the quantitative measurement of MAHA in serum and plasma samples. The assay utilizes the two-site "sandwich" technique with two selected antibodies that bind to MAHA.

Assay standards, controls and patient samples are directly added to wells of a microplate that is coated with highly purified human IgG. After the first incubation period, the MAHA binds to the human IgG on the wall of microtiter well and unbound proteins in each microtiter well are washed away. Then a horseradish peroxidase (HRP) labeled human antibody is added to each microtiter well and a "sandwich" of "well coated human IgG – MAHA – HRP-Conjugated human antibody" is formed. The unbound HRP conjugated human antibody is removed in the subsequent washing step. For the detection of this immunocomplex, the well is then incubated with a substrate solution in a timed reaction and then measured in a spectrophotometric microplate reader. The enzymatic activity of the immunocomplex bound to MAHA on the wall of the microtiter well is directly proportional to the amount of MAHA in the sample. A standard curve is generated by plotting the absorbance versus the respective MAHA concentration for each standard on point-to-point or 4 parameter curve fit. The concentration of MAHA in test samples is determined directly from this standard curve.

### REAGENTS: Preparation and Storage

This test kit must be stored at 2 – 8°C upon receipt. For the expiration date of the kit refer to the label on the kit box. All components are stable until this expiration date.

**Prior to use allow all reagents to come to room temperature.** Reagents from different kit lot numbers should not be combined or interchanged.

#### 1. Human IgG Coated Microplate (Cat. No. 30328)

One well-breakable microplate with 12 x eight strips (96 wells total) coated with highly purified human IgG. The plate is framed and sealed in a foil zipper bag with a desiccant. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

#### 2. HRP Conjugated Human Antibody (Cat. No. 30329)

One vial containing 0.6 mL HRP labeled human antibody in a stabilized protein matrix. This reagent must be diluted with Tracer Antibody Diluent before use. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

### 3. Tracer Antibody Diluent (Cat. No. 30052)

One vial containing 12 mL ready to use buffer. It should be used only for tracer antibody dilution according to the assay procedures. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

### 4. Assay Buffer (Cat. No. 30074)

One bottle containing 30 mL of ready-to-use phosphate buffered saline based assay buffer with bovine serum albumin added. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

### 5. ELISA Wash Concentrate (Cat. No. 10010)

One bottle contains 30 mL of 30 fold concentrate. The contents must be diluted with 870 mL of distilled water prior to use and mix well. Upon dilution this yields a working wash solution containing a surfactant in phosphate buffered saline with a non-azide and non-mercury based preservative. The diluted wash buffer should be stored at room temperature and is stable until the expiration date on the kit box.

### 6. ELISA HRP Substrate (Cat. No. 10020)

One bottle contains 12 mL of tetramethylbenzidine (TMB) with stabilized hydrogen peroxide. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

### 7. ELISA Stop Solution (Cat. No. 10030)

One bottle contains 12 mL of 0.5 M sulfuric acid. This reagent should be stored at 2 – 8°C or room temperature and is stable until the expiration date on the kit box.

### 8. MAHA Standards (Cat. No. 30491 – 30495)

Five vials containing different levels of MAHA in a liquid protein matrix with a non-azide based preservative.

**Refer to vial for exact concentration for each standard.** These reagents should be stored at 2 – 8°C and are stable until the expiration date on the kit box.

### 9. MAHA Controls (Cat. No. 30496 – 30497)

Two vials containing different levels of MAHA in a liquid protein matrix with a non-azide based preservative.

**Refer to vials for exact concentration range for each control.** Both controls should be stored at 2 – 8°C and are stable until the expiration date on the kit box.

## SAFETY PRECAUTIONS

The reagents must be used in a professional laboratory environment and are for research use only. Source material (e.g. highly purified bovine serum albumin) of bovine serum was derived in the contiguous 48 United States. It was obtained only from healthy donor animals maintained under veterinary supervision and found free of contagious diseases. Wear gloves while performing this assay and handle these reagents as if they are potential infectious. Avoid contact with reagents containing TMB, hydrogen peroxide, or sulfuric acid. TMB may cause irritation to skin and mucous membranes and cause an allergic skin reaction. TMB is a suspected carcinogen. Sulfuric acid may cause severe irritation on contact with skin. Do not get in eyes, on skin, or on clothing. Do not ingest or inhale fumes. On contact, flush

with copious amounts of water for at least 15 minutes. Use Good Laboratory Practices.

## MATERIALS REQUIRED BUT NOT PROVIDED

1. Precision single channel pipettes capable of delivering 25  $\mu$ L, 50  $\mu$ L, 100  $\mu$ L, and 1000  $\mu$ L etc.
2. Repeating dispenser suitable for delivering 100  $\mu$ L.
3. Disposable pipette tips suitable for above volume dispensing.
4. Disposable 12 x 75 mm or 13 x 100 glass tubes.
5. Disposable plastic 100 mL and 1000 mL bottle with caps.
6. Aluminum foil.
7. Deionized or distilled water.
8. Plastic microtiter well cover or polyethylene film.
9. ELISA multichannel wash bottle or automatic (semi-automatic) washing system.
10. Spectrophotometric microplate reader capable of reading absorbance at 450 nm.

## SPECIMEN COLLECTION

Only 50  $\mu$ L of mouse serum or plasma is required for MAHA measurement in duplicate. No special preparation of subject is necessary prior to specimen collection. In the case of serum, whole blood should be collected and must be allowed to clot for a minimum of 30 minutes at room temperature before the serum is separated by centrifugation (850 – 1500xg for 10 minutes). The serum should be separated from the clot within three hours of blood collection and transferred to a clean test tube. Serum or plasma samples should be stored at 2 - 8°C if the assay is to be performed within 72 hours. Otherwise, the samples should be stored at - 20°C or below until measurement. Avoid repeated (more than three times) freezing and thawing of specimen.

## ASSAY PROCEDURE

### 1. Reagent Preparation

- (1) Prior to use allow all reagents to come to room temperature. Reagents from different kit lot numbers should not be combined or interchanged.
- (2) ELISA Wash Concentrate (Cat. 10010) must be diluted to working solution prior use. Please see REAGENTS section for details.
- (3) Assay Procedure
  - (1) Place a sufficient number of human IgG coated microwell strips/wells (Cat. 30328) in a holder to run MAHA standards, controls and unknown samples in duplicate.
  - (2) Test Configuration

ROW	STRIP 1	STRIP 2	STRIP 3
A	STD 1	STD 5	SAMPLE 2
B	STD 1	STD 5	SAMPLE 2
C	STD 2	C 1	SAMPLE 3
D	STD 2	C 1	SAMPLE 3
E	STD 3	C 2	SAMPLE 4
F	STD 3	C 2	SAMPLE 4
G	STD 4	SAMPLE 1	
H	STD 4	SAMPLE 1	

- (3) Add **25  $\mu$ L** of standards (Cat. 30491-30495), controls (Cat. 30496-30497) and patient samples into the designated microwell.
- (4) Add **100  $\mu$ L** of assay buffer (Cat. 30074) to each well
- (5) Cover the plate with one plate sealer and incubate plate at room temperature, shaking for **45 minutes**.

- (6) Prepare MAHA tracer antibody working solution by **1:21** fold dilution of the HRP-conjugated human antibody (Cat. 30329) with the tracer Antibody Diluent (Cat. 30052). For each strip, it is required to mix 1 mL of the tracer antibody diluent with 50  $\mu$ L of the tracer antibody in a clean test tube.
- (7) Remove plate sealer. Aspirate the contents of each well. Wash each well 5 times by dispensing 350  $\mu$ L of working wash solution into each well and then completely aspirating the contents. Alternatively, an automated microplate washer can be used.
- (8) Add **100  $\mu$ L** of above diluted MAHA tracer antibody to each of the wells.
- (9) Cover the plate with a plate sealer and an aluminum foil to and incubate plate at room temperature, shaking for **45 minutes**.
- (10) Remove plate sealer. Aspirate the contents of each well. Wash each well 5 times by dispensing 350  $\mu$ L of working wash solution into each well and then completely aspirating the contents. Alternatively, an automated microplate washer can be used.
- (11) Add **100  $\mu$ L** of ELISA HRP Substrate (Cat. 10020) into each of the wells.
- (12) Cover the plate with a plate sealer and also with an aluminum foil to avoid exposure to light.
- (13) Incubate plate at room temperature for **20 minutes**.
- (14) Remove the aluminum foil and plate sealer. Add 100  $\mu$ L of ELISA Stop Solution (Cat. 10030) into each of the wells. Mix gently.
- (15) Read the absorbance at **450 nm** within 10 minutes in a microplate reader.

*NOTE: to reduce the background, one can set the instrument to dual wavelength measurement at 450 nm with background wavelength correction set at 595 nm or 620 nm or 630 nm.*

#### PROCEDURAL NOTES

1. It is recommended that all standards, controls and unknown samples be assayed in duplicate. The average absorbance reading of each duplicate should be used for data reduction and the calculation of results.
2. For mouse samples with concentration higher than level 5 standard, it is recommended to measure diluted the specimen with assay buffer at 1:10, 1:100, etc. for a more accurate report.
3. Keep light sensitive reagents in the original amber bottles.
4. Store any unused human IgG coated strips in the foil Ziploc bag with desiccant to protect from moisture.
5. Careful technique and use of properly calibrated pipetting devices are necessary to ensure reproducibility of the test.
6. Incubation times or temperatures other than those stated in this insert may affect the results.
7. Avoid air bubbles in the microwell as this could result in lower binding efficiency and higher CV% of duplicate reading.
8. All reagents should be mixed gently and thoroughly prior use. Avoid foaming.

#### INTERPRETATION OF RESULTS

1. Calculate the average absorbance for each pair of duplicate test results.
2. Subtract the average absorbance of the STD 1 (0  $\mu$ g/mL ) from the average absorbance of all other readings to obtain corrected absorbance.
3. The standard curve is generated by the corrected absorbances of all standard levels on the ordinate against the standard concentration on the abscissa using point-to-point or log-log paper. Appropriate computer assisted data reduction programs may also be used for the calculation of results. We recommend using **Point-to-Point** curve fit.


The MAHA concentrations for the controls and test samples are read directly from the standard curve using their respective corrected absorbance.

#### EXAMPLE DATA AND STANDARD CURVE

A typical absorbance data and the resulting standard curve from this MAMA ELISA are represented. **This curve should not be used in lieu of standard curve run with each assay.**

Well I.D.	OD 450 nm Absorbance			Results $\mu$ g/mL
	Readings	Average	Corrected	
0 $\mu$ g/mL	0.047 0.046	0.047	0.000	
1 $\mu$ g/mL	0.342 0.338	0.340	0.293	
3 $\mu$ g/mL	1.178 1.094	1.136	1.089	
9 $\mu$ g/mL	2.501 2.336	2.418	2.371	
27 $\mu$ g/mL	3.224 3.205	3.214	3.167	
Control 1	0.598 0.643	0.620	0.573	1.71 $\mu$ g/mL
Control 2	1.988 2.013	2.000	1.953	7.04 $\mu$ g/mL

## MAHA ELISA

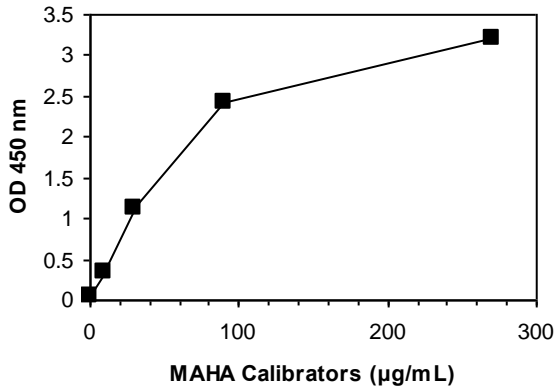

### EXPECTED VALUES

Normal mouse sera were measured with this MAHA ELISA. The 99% confidence normal cut-off is **0.5 µg/mL**.

It is highly recommend that each laboratory establish its own normal cut off level or establish a baseline MAHA value before injection of humanized monoclonal antibody to the study animal.

### LIMITATION OF THE PROCEDURE

1. Since this is the first commercial assay of this kind and there is no Gold Standard concentration or international standard available for MAHA measurement, the values of assay standards were established and validated by Epitepe Diagnostics. Results obtained with different assay methods or kits cannot be used interchangeably.
2. For unknown sample value read directly from the assay that is greater than the highest assay standard, it is recommend measuring a further diluted sample for more accurate measurement.
3. Bacterial or fungal contamination of serum specimens or reagents, or cross contamination between reagents may cause erroneous results.
4. Water deionized with polyester resins may inactivate the horseradish peroxidase enzyme.

### QUALITY CONTROL

To assure the validity of the results each assay should include adequate controls with known MAHA levels. We recommend that all assays include the laboratory's own MAHA controls in addition to those provided with this kit.

### PERFORMANCE CHARACTERISTICS

#### Sensitivity

The sensitivity of this MAHA ELISA as determined by the 95% confidence limit on 20 duplicate determination of zero standard is about **0.1 µg/mL**.

### High Dose "hook" effect

This assay has showed that it did not have any high dose "hook" effect up to 3,000 µg/mL.

### Precision

The intra-assay precision was validated by measuring one control sample in a single assay with eight replicate determinations.

Mean MAHA Value (µg/mL)	CV (%)
1.62	5.1

The inter-assay precision is validated by measuring one control sample in duplicate in 6 individual assays.

Mean MAHA Value (µg/mL)	CV (%)
6.93	6.7

### WARRANTY

This product is warranted to perform as described in its labeling and literature when used in accordance with all instructions. Epitepe Diagnostics, Inc. DISCLAIMS ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE, and in no event shall Epitepe Diagnostics, Inc. be liable for consequential damages. Replacement of the product or refund of the purchase price is the exclusive remedy for the purchaser. This warranty gives you specific legal rights and you may have other rights, which vary from state to state.

### Other Related Products:

1. HAAH (Human Anti-Human Antibody) ELISA Kit, Cat# KT-806
2. HAMA (Human Anti-Mouse Antibody) ELISA Kit, Cat# KT-805


### REFERENCES

1. Szolar OH, Stranner S, Zinoecker I, Mudde GC, Himmler G, Waxenecker G, Nechansky A. Qualification and application of a surface plasmon resonance-based assay for monitoring potential HAAH responses induced after passive administration of a humanized anti Lewis-Y antibody. J Pharm Biomed Anal. 2006 Jun 16;41(4):1347-53. Epub 2006 Apr 27
2. Ritter G, Cohen LS, Williams C Jr, Richards EC, Old LJ, Welt S. Serological analysis of human anti-human antibody responses in colon cancer patients treated with repeated doses of humanized monoclonal antibody A33. Cancer Res. 2001 Sep 15;61(18):6851-9
3. Lofgren JA, Dhandapani S, Pennucci JJ, Abbott CM, Mytych DT, Kaliyaperumal A, Swanson SJ, Mullenix MC. Comparing ELISA and surface plasmon resonance for assessing clinical immunogenicity of panitumumab. J Immunol. 2007 Jun 1;178(11):7467-72
4. Szolar OH, Stranner S, Zinoecker I, Mudde GC, Himmler G, Waxenecker G, Nechansky A. Qualification and application of a surface plasmon resonance-based assay for monitoring potential HAAH responses induced after passive administration of a humanized anti Lewis-Y antibody. J Pharm Biomed Anal. 2006 Jun 16;41(4):1347-53. Epub 2006 Apr 27










**TECHNICAL ASSISTANCE AND CUSTOMER SERVICE**

For technical assistance or place an order, please contact Epitope Diagnostics, Inc. at (858) 693-7877 or fax to (858) 693-7678. [www.epitopediagnostics.com](http://www.epitopediagnostics.com)

This product is developed and manufactured by

 **Epitope Diagnostics, Inc.**  
San Diego, CA 92121, USA

- Add 25 µl of standards, control and mouse sample to the plate
  - Add 100 µl of assay buffer
  - Incubate 45 min at RT, shaking
  - Wash strips with diluted wash buffer
  - Add 100 µl MAHA Tracer Antibody
  - Incubate 45 min at RT, shaking
  - Wash strips with diluted wash buffer
  - Add 100 µl TMB substrate
  - Incubate 20 min at RT
  - Add 100 µl stop solution
  - Read strips at OD 450 nm
- 

 Manufacturer	 No. of tests
 Catalog Number	 Keep away from heat and direct sun light
 Concentrate	 Store at
 Read instructions before use	 Use by
	 Lot No.

---

**Short Assay Protocol:**